
Data File C:\CHEM32\1\DATA\SIG10228.D
Sample Name: 100SV076 LOTE 047/26

```
==========================================================================
Acq. Operator   : Anderson
Acq. Instrument : Instrument 1                    Location : Vial 1
Injection Date  : 16/10/2026 09:07:08                  Inj :   1
                                                 Inj Volume : Manually
Acq. Method     : C:\CHEM32\1\METHODS\2026ATUAL.M
Last changed    : 16/10/2026 08:18:14 by Anderson
Analysis Method : C:\CHEM32\1\METHODS\2026ATUAL.M
Last changed    : 16/10/2026 09:55:52 by Anderson
                  (modified after loading)
Sample Info     : 100SV076 LOTE 047/26


Sample-related custom fields:

Name                           |Value
-------------------------------|--------------------------------------
Additional Info : Peak(s) manually integrated
```

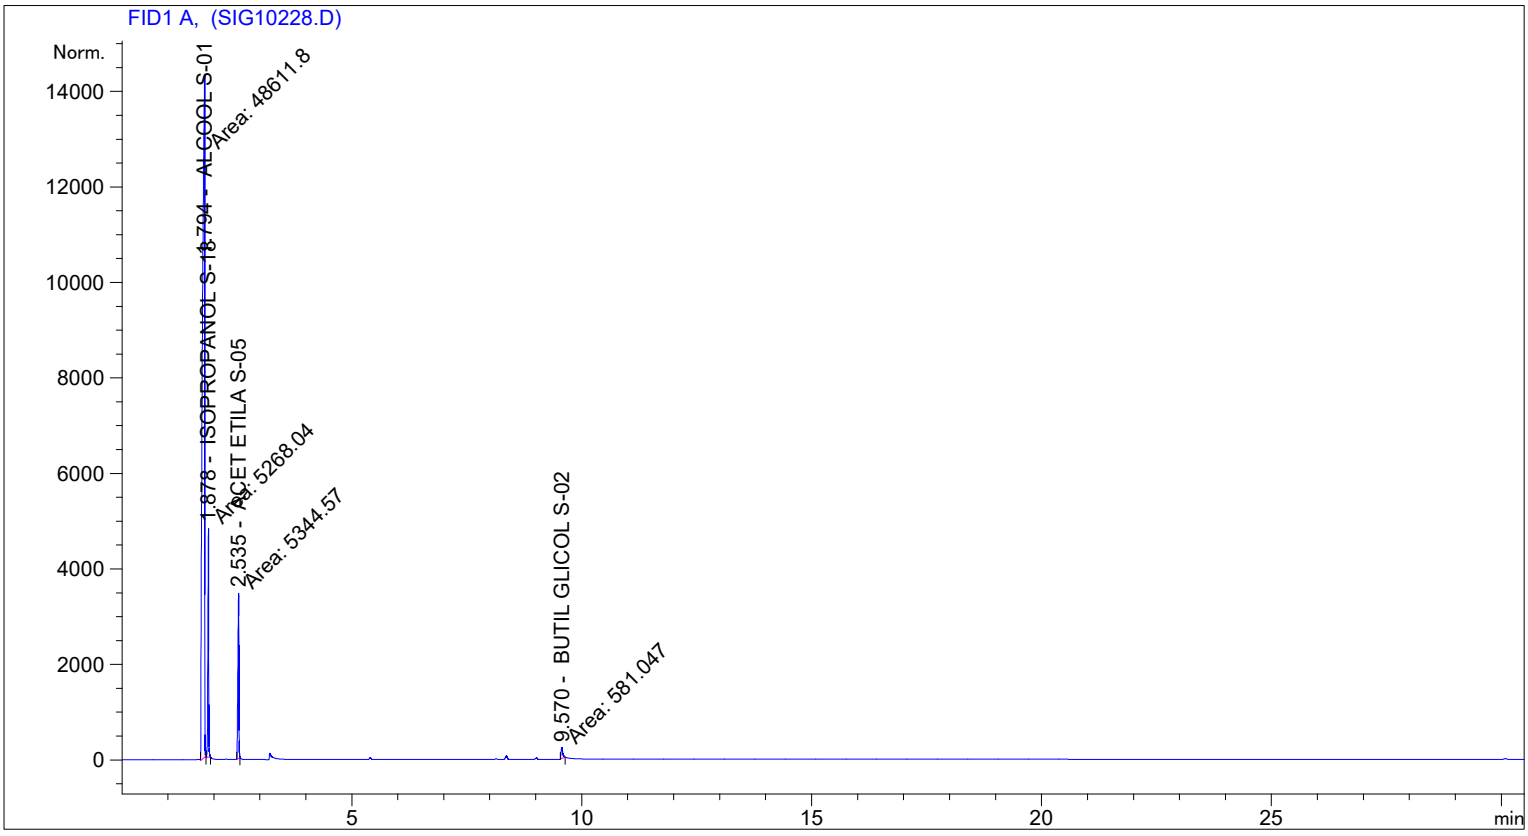


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      16/10/2026 09:56:23
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: FID1 A,

Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [pA*s]        %
----|-------|------|-------|----------|--------|--------------------
   1   0.000         0.0000    0.00000  0.00000
   2   0.000         0.0000    0.00000  0.00000
   3   1.730         0.0000    0.00000  0.00000 ALCOOL S-01
```

Data File C:\CHEM32\1\DATA\SIG10228.D
Sample Name: 100SV076 LOTE 047/26

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
4	1.746		0.0000	0.00000	0.00000	ALCOOL S-01
5	1.794	MM	0.0557	4.86118e4	81.28320	ALCOOL S-01
6	1.830		0.0000	0.00000	0.00000	ACETONA S-08
7	1.878	MM	0.0183	5268.04150	8.80863	ISOPROPANOL S-18
8	2.390		0.0000	0.00000	0.00000	HEXANO S-96
9	2.500		0.0000	0.00000	0.00000	MEK S-09
10	2.535	MM	0.0257	5344.57324	8.93660	ACET ETILA S-05
11	3.000		0.0000	0.00000	0.00000	ISOBUTANOL S-20
12	3.870		0.0000	0.00000	0.00000	DOWANOL PM S-24
13	4.930		0.0000	0.00000	0.00000	ETIL GLICOL S-17
14	5.170		0.0000	0.00000	0.00000	MIBK S-16
15	5.700		0.0000	0.00000	0.00000	TOLUOL S-07
16	6.398		0.0000	0.00000	0.00000	ACETATO DE BUTILA S-32
17	7.827		0.0000	0.00000	0.00000	DIACETONA ALCOOL S-31
18	8.066		0.0000	0.00000	0.00000	ACET AMILA S-15
19	8.290		0.0000	0.00000	0.00000	XILOL S-06
20	8.744		0.0000	0.00000	0.00000	ACET ETIL GLICOL S-34
21	9.570	MM	0.0422	581.04712	0.97156	BUTIL GLICOL S-02
22	11.940		0.0000	0.00000	0.00000	AB9 S-12

Totals : 5.98054e4

6 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)
Warning : Calibrated compound(s) not found
Warning : Invalid calibration curve, (ALCOOL S-01)
Warning : Invalid calibration curve, (ISOPROPANOL S-18)
Warning : Invalid calibration curve, (ACET ETILA S-05)
Warning : Invalid calibration curve, (BUTIL GLICOL S-02)

==========

*** End of Report ***