
Data File C:\CHEM32\1\DATA\SIG10227.D
Sample Name: THINNER ALV

```
==========================================================================
Acq. Operator    : Anderson
Acq. Instrument  : Instrument 1                    Location : Vial 1
Injection Date   : 13/10/2026 14:02:58                  Inj :   1
                                                  Inj Volume : Manually
Acq. Method      : C:\CHEM32\1\METHODS\2026ATUAL.M
Last changed     : 13/10/2026 09:06:03 by Anderson
Analysis Method  : C:\CHEM32\1\METHODS\2026ATUAL.M
Last changed     : 13/10/2026 14:33:30 by Anderson
Sample Info      : THINNER ALV


Sample-related custom fields:

Name                           |Value
-------------------------------|-------------------------------------
Additional Info : Peak(s) manually integrated
```

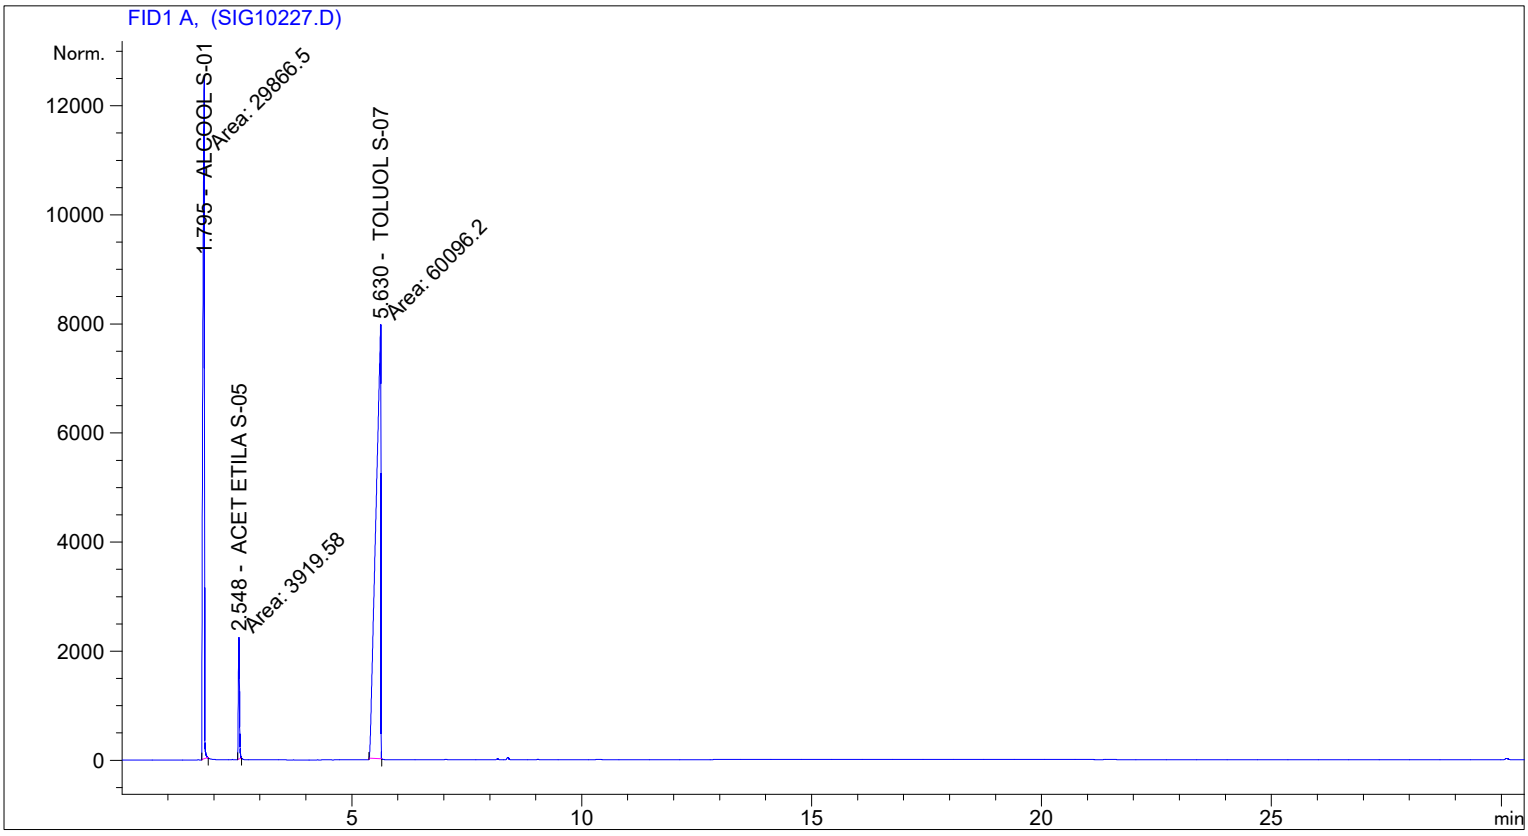


```
==========================================================================
                          Area Percent Report
==========================================================================

Sorted By             :      Signal
Calib. Data Modified  :      09/10/2026 11:19:41
Multiplier            :      1.0000
Dilution              :      1.0000
Use Multiplier & Dilution Factor with ISTDs


Signal 1: FID1 A,

Peak RetTime  Type   Width     Area      Area    Name
  #   [min]          [min]   [pA*s]        %
----|-------|------|-------|----------|--------|--------------------
   1   0.000         0.0000    0.00000  0.00000
   2   0.000         0.0000    0.00000  0.00000
   3   1.730         0.0000    0.00000  0.00000 ALCOOL S-01
   4   1.746         0.0000    0.00000  0.00000 ALCOOL S-01
```

Data File C:\CHEM32\1\DATA\SIG10227.D
Sample Name: THINNER ALV

| Peak # | RetTime [min] | Type | Width [min] | Area [pA*s] | Area % | Name |
|---|---|---|---|---|---|---|
| 5 | 1.795 | MM | 0.0390 | 2.98665e4 | 31.81273 | ALCOOL S-01 |
| 6 | 1.830 | | 0.0000 | 0.00000 | 0.00000 | ACETONA S-08 |
| 7 | 1.890 | | 0.0000 | 0.00000 | 0.00000 | ISOPROPANOL S-18 |
| 8 | 2.390 | | 0.0000 | 0.00000 | 0.00000 | HEXANO S-96 |
| 9 | 2.500 | | 0.0000 | 0.00000 | 0.00000 | MEK S-09 |
| 10 | 2.548 | MM | 0.0293 | 3919.58032 | 4.17499 | ACET ETILA S-05 |
| 11 | 3.000 | | 0.0000 | 0.00000 | 0.00000 | ISOBUTANOL S-20 |
| 12 | 3.870 | | 0.0000 | 0.00000 | 0.00000 | DOWANOL PM S-24 |
| 13 | 4.930 | | 0.0000 | 0.00000 | 0.00000 | ETIL GLICOL S-17 |
| 14 | 5.170 | | 0.0000 | 0.00000 | 0.00000 | MIBK S-16 |
| 15 | 5.630 | MM | 0.1258 | 6.00962e4 | 64.01228 | TOLUOL S-07 |
| 16 | 6.398 | | 0.0000 | 0.00000 | 0.00000 | ACETATO DE BUTILA S-32 |
| 17 | 7.827 | | 0.0000 | 0.00000 | 0.00000 | DIACETONA ALCOOL S-31 |
| 18 | 8.066 | | 0.0000 | 0.00000 | 0.00000 | ACET AMILA S-15 |
| 19 | 8.290 | | 0.0000 | 0.00000 | 0.00000 | XILOL S-06 |
| 20 | 8.744 | | 0.0000 | 0.00000 | 0.00000 | ACET ETIL GLICOL S-34 |
| 21 | 8.908 | | 0.0000 | 0.00000 | 0.00000 | BUTIL GLICOL S-02 |
| 22 | 11.940 | | 0.0000 | 0.00000 | 0.00000 | AB9 S-12 |

Totals : 9.38823e4

5 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)
Warning : Calibrated compound(s) not found
Warning : Invalid calibration curve, (ALCOOL S-01)
Warning : Invalid calibration curve, (ACET ETILA S-05)
Warning : Invalid calibration curve, (TOLUOL S-07)

==========

*** End of Report ***